



Appn No.: 10/669,059

Applicant(s): Schoenle et al.

MEDICAL DEVICE COMPONENTS AND PROCESSES

Reply to Notice of Non-Compliant Amend. of Dec. 22, 2004

Replacement Sheet

Page 1 of 5

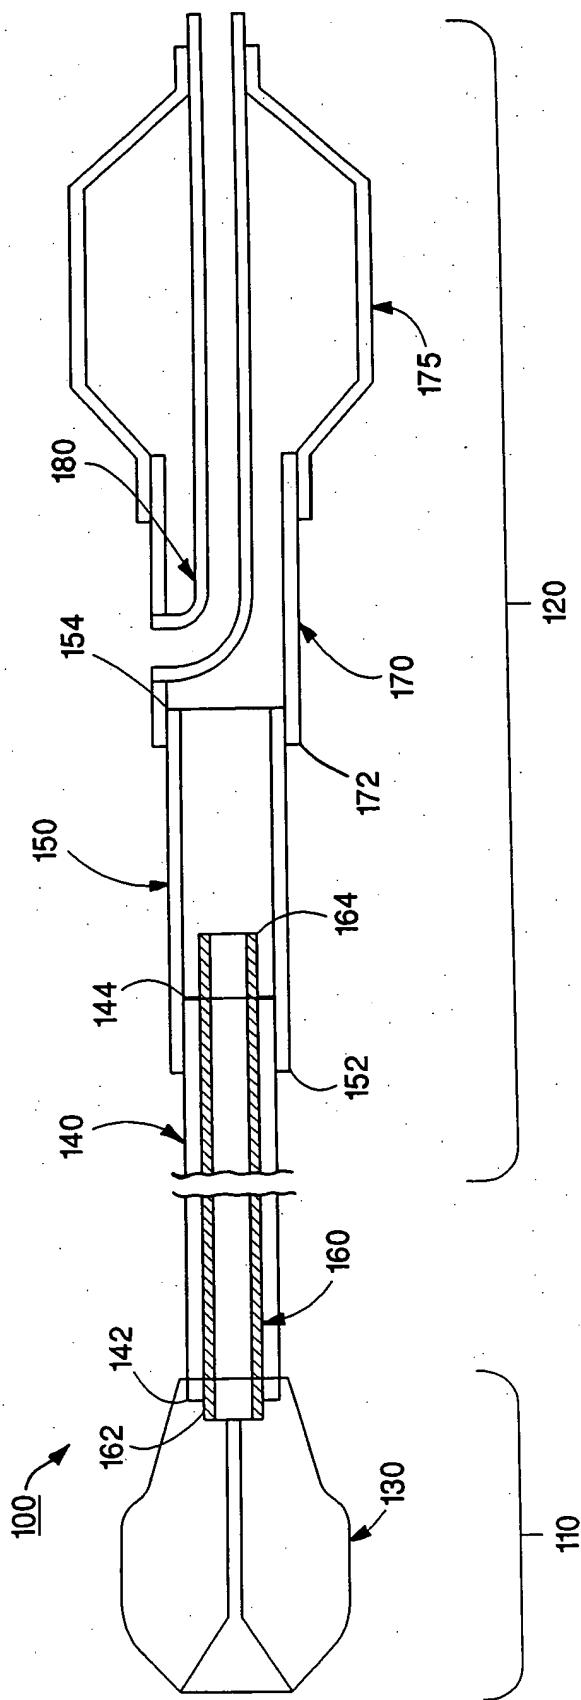


FIG. 1

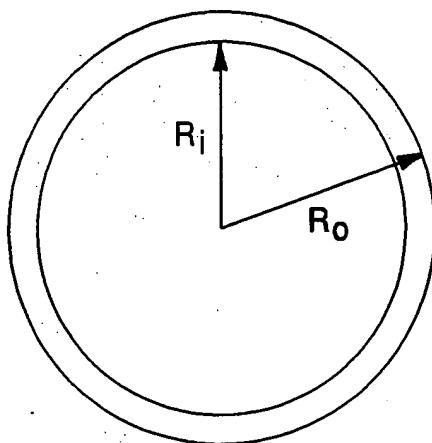


FIG. 2

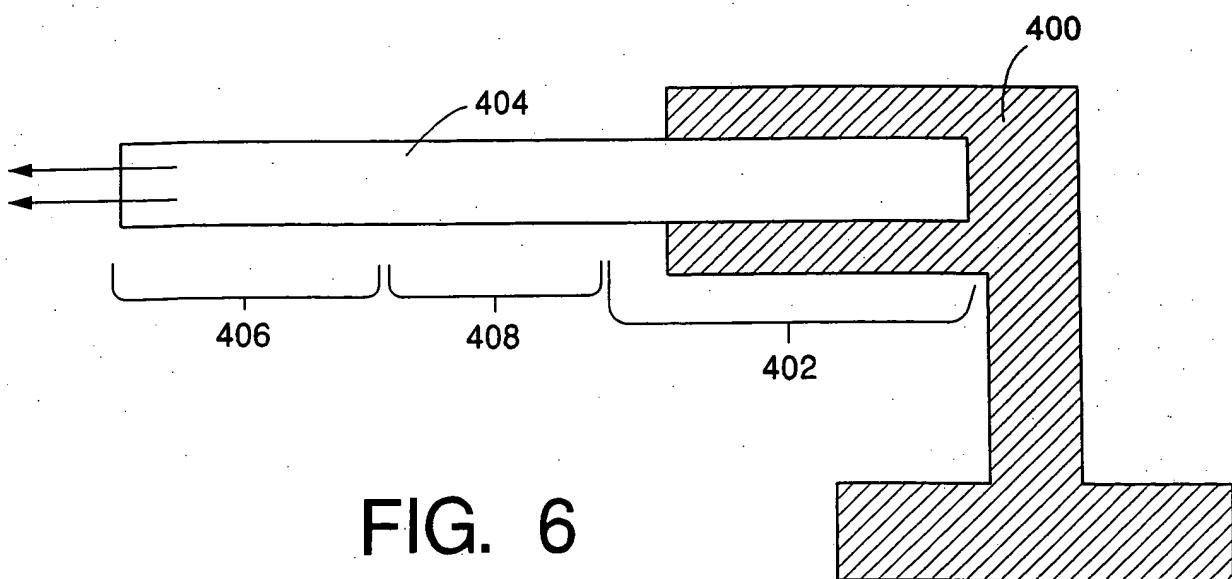
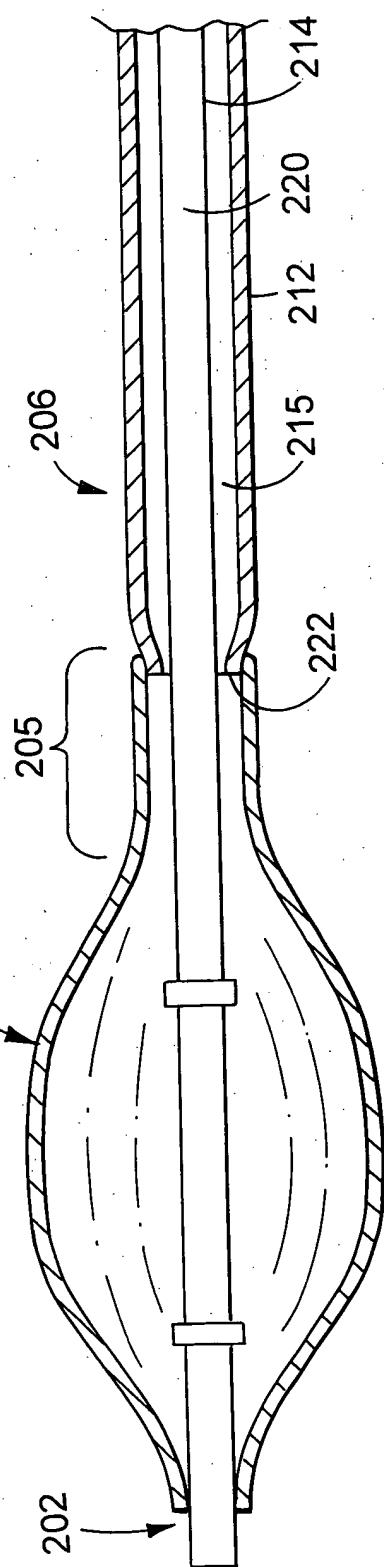
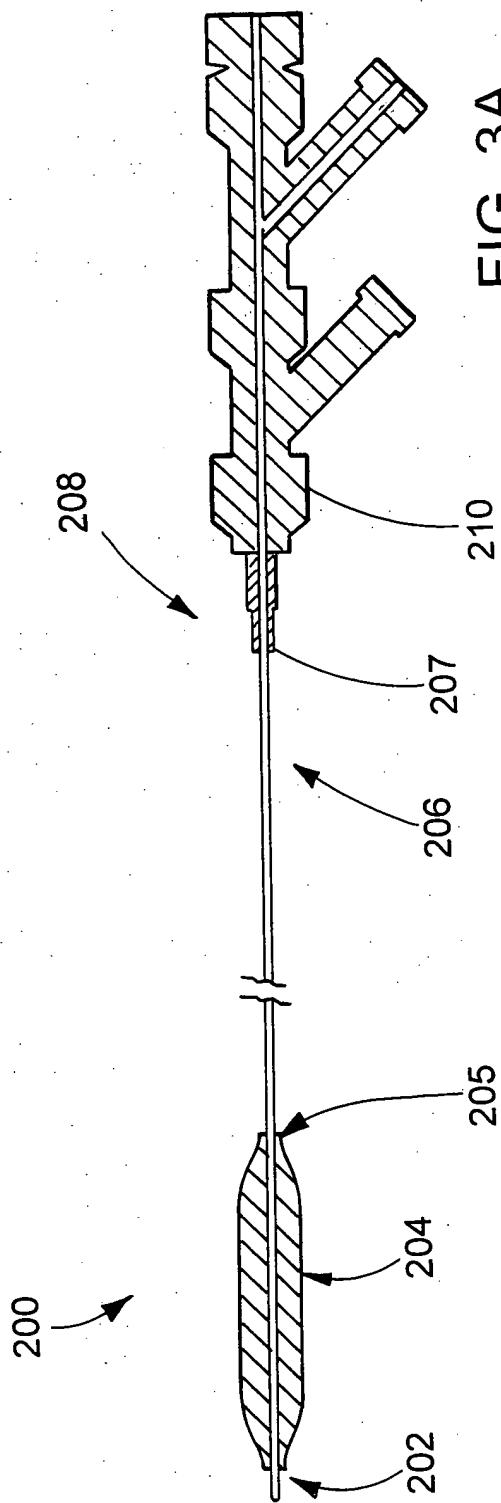


FIG. 6










FIG. 4A  
300

FIG. 4B


FIG. 4C  
310FIG. 4D  
310FIG. 4E  
320




**FIG. 5A**

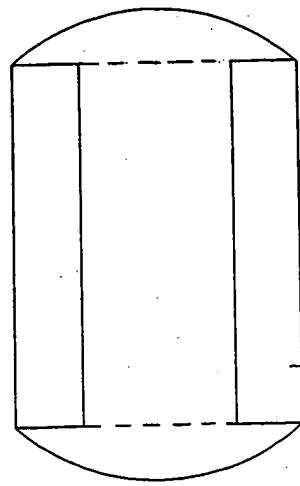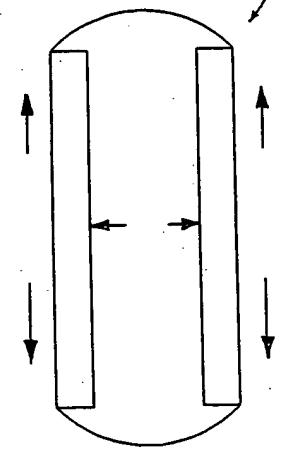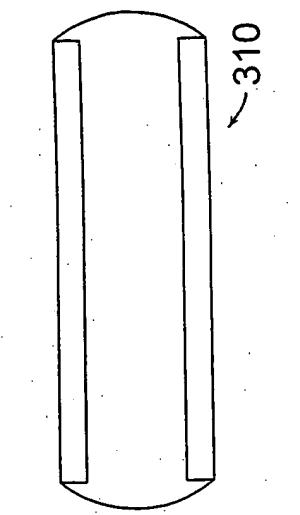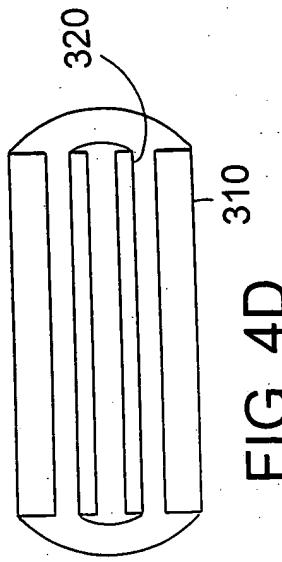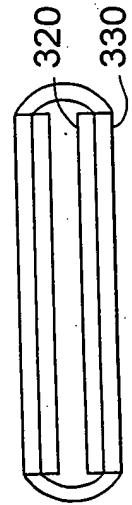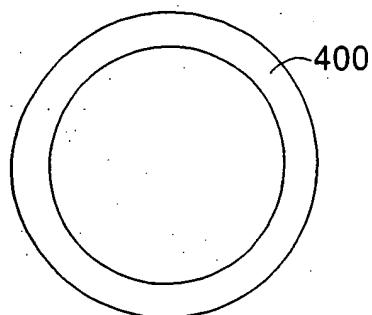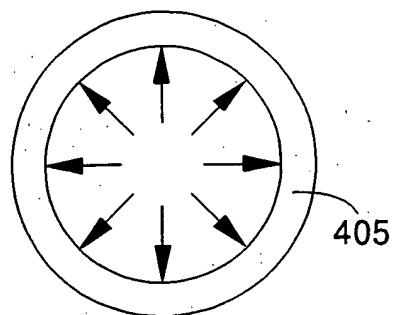


**FIG. 5B**

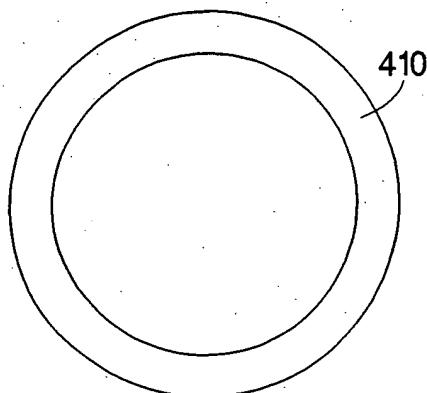

**FIG. 5C**

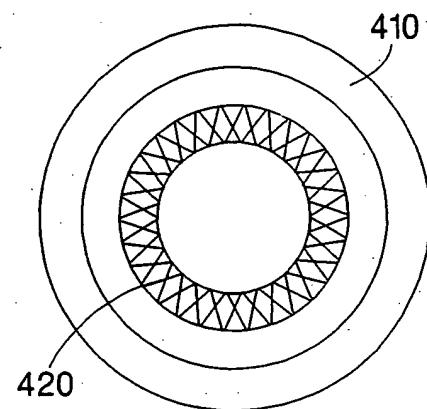

**FIG. 5D**

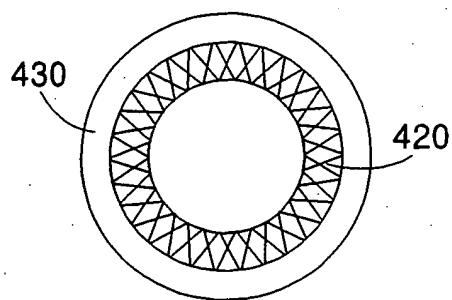

**FIG. 5E**